Fig. 1

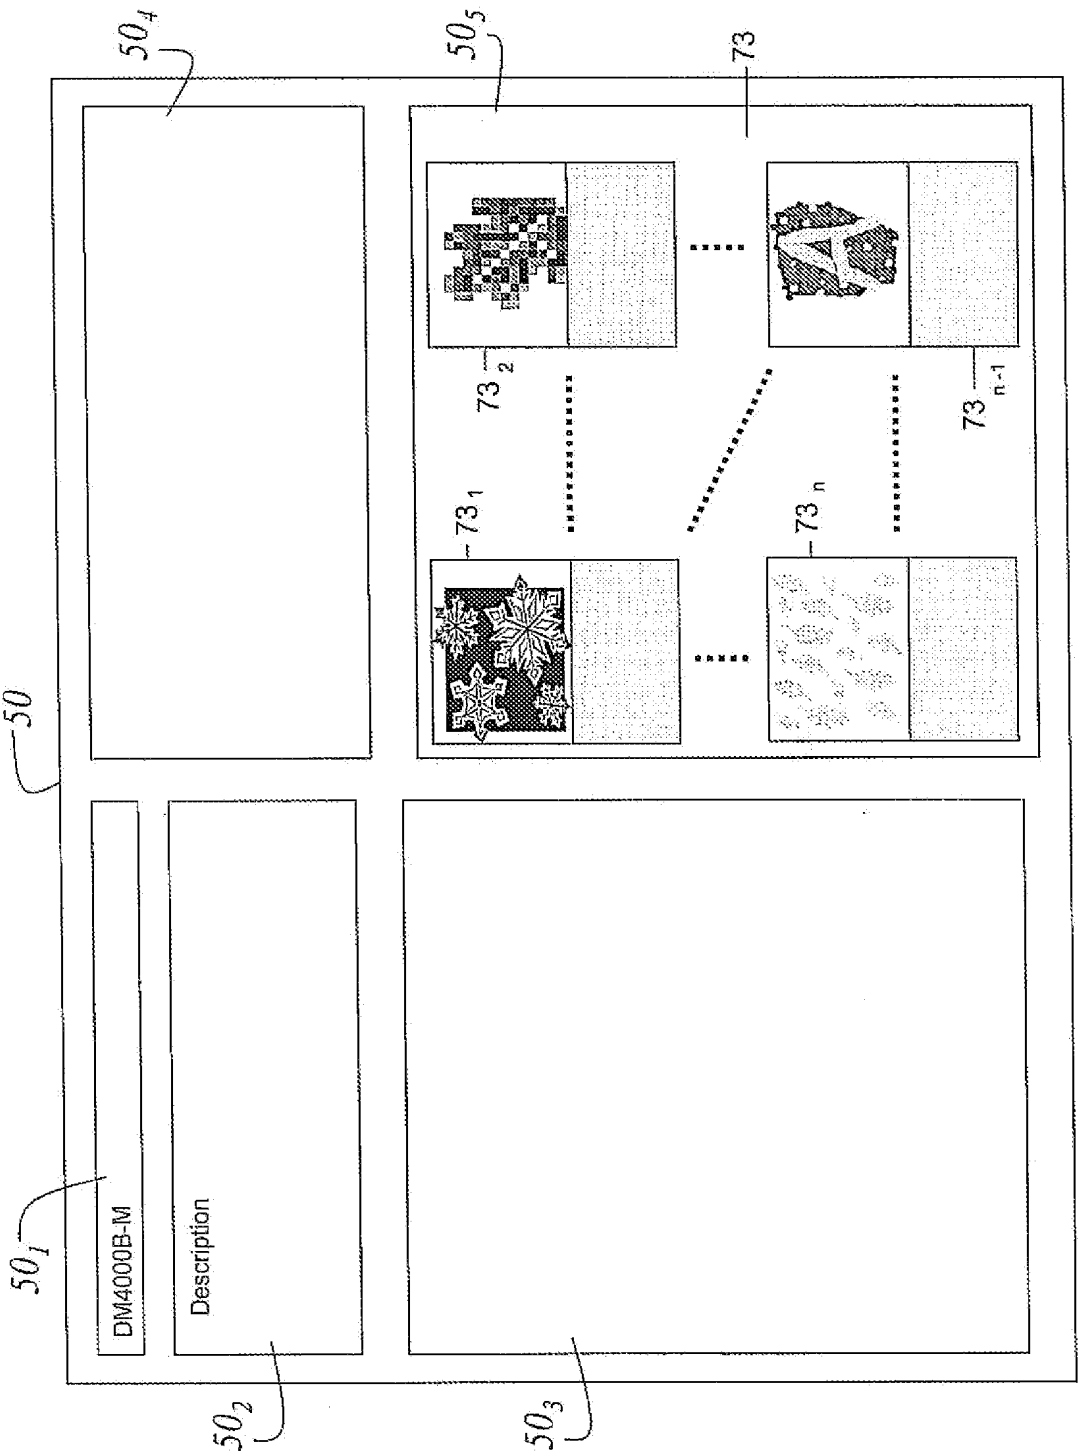


Fig. 2

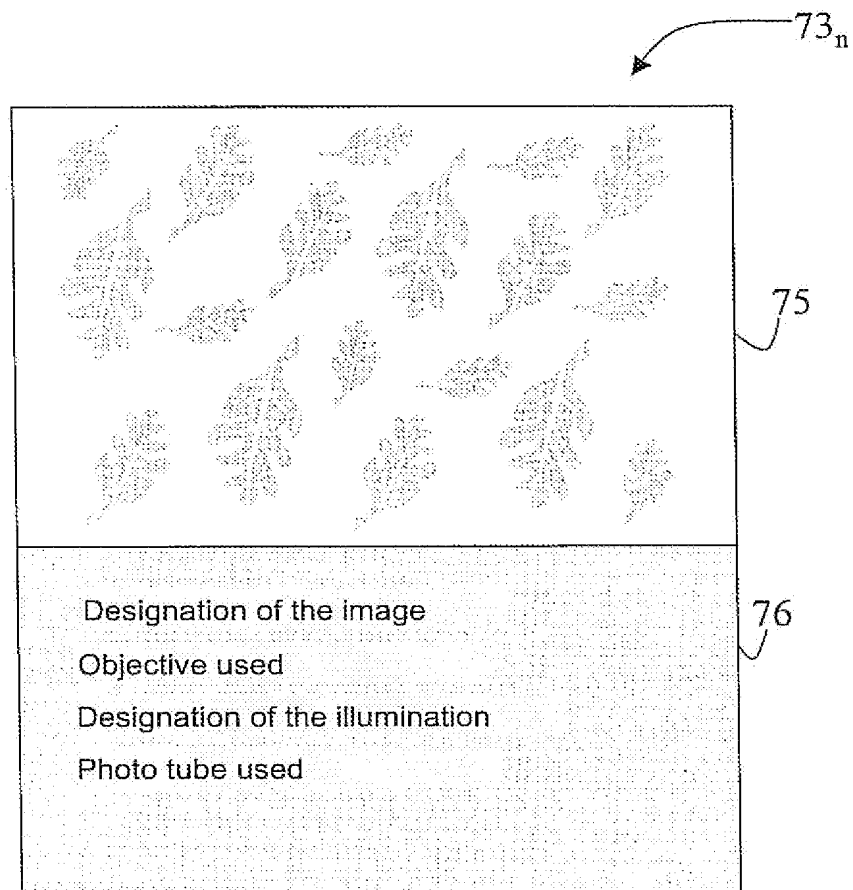


Fig. 4

90

91 92

Property	Status
CONTRASTING_METHOD	OK
MICROSCOPE_NOSEPIECE	not set
MICROSCOPE_MAGNIFICATION_CHANGER	not implemented
MICROSCOPE_LAMP	OK
MICROSCOPE_TL_FIELD_DIAPHRAGM	OK
MICROSCOPE_TL_APERTURE_DIAPHRAGM	OK
MICROSCOPE_TL_SHUTTER	OK

Fig. 6

101 100 102

Property	Status
<div>103 OK</div> <div>104 Cancel</div>	
X value	<input checked="" type="checkbox"/>
Y value	<input checked="" type="checkbox"/>
Z value	<input checked="" type="checkbox"/>

105 ☒

Fig. 7